

# DepleteX<sup>®</sup> Mito DNA Depletion Kit

KIT2002

For post-library depletion of Illumina NGS libraries

## Contents

<b>Product Overview</b> .....	<b>2</b>
Workflow .....	3
Kit Contents and Storage .....	4
Required Materials and Equipment .....	5
Best Practices .....	6
Revision Log .....	6
Input Material .....	7
<b>Protocol</b> .....	<b>8</b>
Step A: Depletion of Mitochondrial DNA .....	8
Step B: PCR Amplification .....	10
<b>Subsequent Steps</b> .....	<b>11</b>

## Contact Us

If you have any questions, contact Technical Support at [support@jumpcodegenomics.com](mailto:support@jumpcodegenomics.com) Find us at our website: [jumpcodegenomics.com](http://jumpcodegenomics.com)

Call us at 1.619.900.1701


## Product Overview

The DepleteX<sup>®</sup> Mito DNA Depletion Kit targets DNA molecules derived from the human mitochondrial chromosome for removal from next generation sequencing (NGS) libraries. The kit leverages the CRISPR Cas9 endonuclease and its associated guide RNA to target and cleave human mitochondrial sequences. In samples with high mitochondrial content, such as ATAC-Seq libraries, use of the DepleteX Mito DNA Depletion Kit maximizes the re-assignment of sequencing reads to informative nuclear content and increases sequencing coverage of DNA derived from the nuclear fraction.

Description	
Total Assay Time	~3 hours
Hands-on Time	~1 hour
Samples Per Kit	24 samples
Sample Type	Human DNA NGS Library *
DNA Library Input	10 ng
DNA Library Size	≥ 200 bp
Designed to Deplete	Human mitochondrial DNA
Method	CRISPR-Cas9 mediated depletion
Validated Library Prep	NEBNext <sup>®</sup> Ultra II FS DNA Library Prep Kit

\* Human RNA NGS libraries with abundant mitochondrial content can also be used as input (see page 7 for more information)

## Workflow

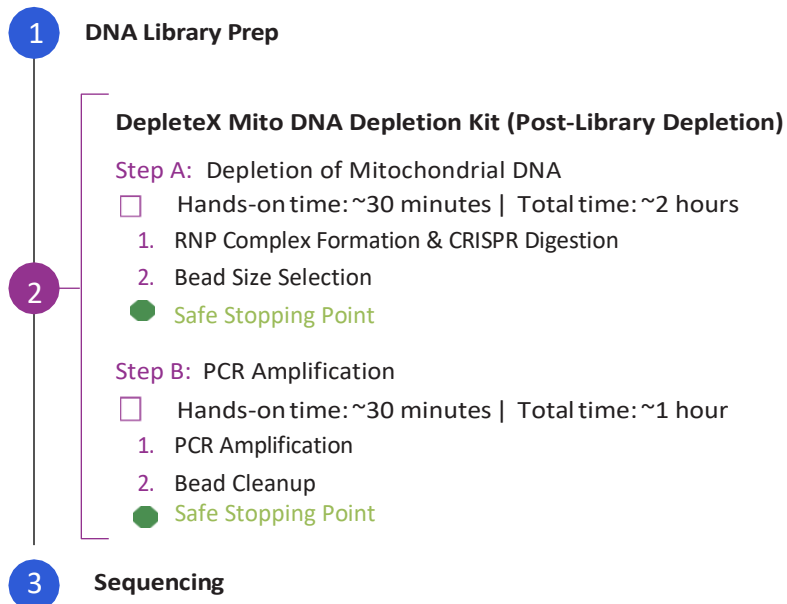

## Kit Contents and Storage

The DepleteX Mito DNA Depletion Kit contains enough material to deplete 24 NGS libraries. The kit contents and storage temperatures are indicated in the tables below.

### ASY1064: Depletion Reagents (8 depletion reactions per box)

3 boxes

Storage at -20°C

Kit contents	Part number	Quantity per box
Cas9	REA1039	1 tube
10X Cas9 Buffer	REA1040	1 tube
RNase Inhibitor	REA1041	1 tube
Nuclease-Free Water	REA1042	1 tube
Tris Buffer	REA1043	1 tube
P5 Primer	REA1044	1 tube
P7 Primer	REA1045	1 tube
2X PCR Mix	REA1046	1 tube

### ASY1069: Guide RNA for Mito DNA Depletion

1 Bag

Storage at -80°C

Kit contents	Part number	Quantity per bag
Mito DNA Guide RNA	REA1052	1 tube

## Required Materials and Equipment

Type	Item	Supplier
Plastic Consumables	0.5 mL, 1.5 mL DNA LoBind Tubes	Eppendorf (Cat# 022431021)
	0.2 mL thin wall PCR tubes	General Lab Supplier
	Low-Retention, Filtered, Sterile Tips (10 µL, 20 µL, 200 µL and 1000 µL)	General Lab Supplier
Reagents	AMPure XP Beads	Beckman Coulter (Cat# A63881)
	Absolute Ethanol, 200 Proof	General Lab Supplier
	Qubit dsDNA HS Assay Kit	ThermoFisher Scientific (Cat# Q32854)
Equipment	Single Channel Pipettes (10 µL, 20 µL, 200 µL, and 1000 µL)	General Lab Supplier
	Multichannel Pipettes (10 µL, 20 µL, and 200 µL)	General Lab Supplier
	Vortex Mixer	General Lab Supplier
	Microcentrifuge	General Lab Supplier
	PCR Magnetic Rack or Stand	General Lab Supplier
	Ice Bucket	General Lab Supplier
	PCR Thermal Cycler	General Lab Supplier
	Qubit Fluorometer	ThermoFisher Scientific (Cat# Q33238)
Automated electrophoresis Instrument such as Agilent TapeStation or 2100 BioAnalyzer	General Lab Supplier	

## Best Practices

### General

- Periodically, optimizations and revisions are made to the kit components and user manual. Therefore, following the protocol included with or appropriate for the kit in question is important. This can be done by comparing the name and version number of the product to the name and version number of the protocol. If you need further assistance in this regard, please contact [support@jumpcodegenomics.com](mailto:support@jumpcodegenomics.com)
- Use properly calibrated pipettes as library preparation is sensitive to pipetting error.
- Follow good laboratory practices throughout the protocol, including RNA-safe procedures when handling RNA. Ensure all pipette tips, microcentrifuge tubes, and other consumables are DNase- and RNase-free.
- When undertaking the protocol, always proceed immediately to the next step. If a stop is necessary, safe stopping points are available. Refer to the workflow schematic on page 3.

### Reagent Handling

- Do not remove Cas9 and RNase Inhibitor from storage until before use. Maintain on ice during reaction setup. Return to -20°C immediately after use.
- Do not remove the guide RNA from storage until immediately before use. Maintain on ice during reaction setup. Return to -80°C immediately after use.
- We recommend a maximum of three freeze-thaw cycles for the guide RNA. It is strongly recommended that multiple smaller aliquots of the guide RNA be prepared when the reagent is first thawed if more than three freeze-thaw cycles are expected.
- Do not freeze AMPure® XP beads.
- Allow AMPure XP beads to come to room temperature before use. A 30-minute incubation on the laboratory bench is usually sufficient.
- Vortex AMPure XP beads immediately before use. Ensure that the beads are in a uniform suspension before use.
- Use magnetic stands appropriate for PCR tubes.

### Equipment Handling

- Thermal cycling should be performed with a heated lid, except where specified otherwise. Thermal cycler(s) must support uniform heating up to 100 µL sample volume.

## Revision Log

Version	Date	Description
v1.0	April 2024	Launch
v1.1	May 2024	Edited for formatting and clarity

## Input Material

Please review and follow the guidelines below for preparing DNA-Seq libraries that are optimal for depletion:

The DepleteX Mito DNA Depletion Kit is optimized for 10 ng of NGS library material. Efficient depletion rates and high-quality NGS data have been validated with the use of the NEBNext® Ultra II FS DNA Library Prep Kit (Cat# E7805).

The DepleteX Mito DNA Depletion Kit can also be used to deplete mitochondrial sequences from RNA-Seq libraries that contain a high proportion of transcripts derived from the mitochondrial genome. Since depletion occurs downstream of library preparation, the protocol for depletion is the same whether NGS libraries are derived from cellular DNA or RNA.

Accurate DNA quality assessment is recommended to maximize depletion efficiency and the efficiency of downstream steps. Validate input DNA using a fluorometric based method, such as a Qubit Fluorometer. Evaluate quality using an automated electrophoresis method, such as the Agilent Bioanalyzer System with a High Sensitivity DNA reagent kit.

### Before Proceeding to Step A.

Please follow the guidelines below:

- Review the library preparation method(s). The libraries should have been prepared and stored under nuclease-free conditions.
- Ensure that the libraries are uniquely indexed.

## Protocol

### Step A: Depletion of Mitochondrial DNA

Hands-on time: ~ 30 min | Total time: ~2 hours

#### Reagent Preparation

Item	Storage	Handling
DNA Library ≥ 200bp (10 ng)	-20°C	If frozen, thaw on ice. Finger-tap mix and spin down. Keep on ice. Return to freezer immediately after use.
Cas9		
RNase Inhibitor		
Mito DNA Guide RNA	-80°C	
Nuclease-Free Water	-20°C	Thaw at room temperature. Vortex briefly and spin down. Keep on ice.
10X Cas9 Buffer		
AMPure XP Beads	4°C	Bring to room temperature. Vortex to mix.
80% Ethanol	Room Temperature	Prepare fresh.

#### A1: Ribonucleoprotein (RNP) Complex Formation and CRISPR Digestion

- Dilute the NGS libraries intended for depletion to a final quantity of 10 ng in 9 µL using Nuclease-Free Water. Set aside for CRISPR digestion (Step A1.5).
- At room temperature, combine the following reagents in the order listed below in a 0.2 mL nuclease-free PCR tube:

RNP Complex Formation Reaction	Volume
Nuclease-Free Water	5.2 µL
10X Cas9 Buffer	1.0 µL
Cas9	1.0 µL
RNase Inhibitor	1.0 µL
Mito DNA Guide RNA	1.8 µL
<b>Total Volume</b>	<b>10 µL</b>

**IMPORTANT:** Keep Cas9 and RNase Inhibitor on ice or in a benchtop cooler when in use. Return the enzymes to the -20°C freezer immediately after use. Return the guide RNA stock to the -80°C freezer immediately after use.

- Mix gently by flicking the tube or pipetting up and down. Collect the contents at the bottom of the tube by briefly spinning the tube in a microcentrifuge.
- Incubate the reaction mix at room temperature for 10 minutes. This constitutes the “Ribonucleoprotein (RNP) Complex.”
- To the tube containing the RNP complex, add the following reagents in the order listed below at room temperature:

CRISPR Digestion Reaction	Volume
RNP Complex (Previous Step A1.4)	10 µL
DNA Library (10 ng)	9 µL
10X Cas9 Buffer	1 µL
<b>Total Volume</b>	<b>20 µL</b>

- Mix gently by flicking the tube or pipetting up and down slowly. Collect the contents at the bottom of the tube by briefly spinning the tube in a microcentrifuge.



- Place the tube in a thermal cycler with a heated lid set to  $\geq 80^{\circ}\text{C}$ . Run the following program:

Temperature	Cycle Time
37°C	16 hours
4°C	HOLD

- Following incubation, proceed to the next step (Bead Size Selection).

**A2: Bead Size Selection**

- Add 30  $\mu\text{L}$  of Nuclease-Free Water to the CRISPR digestion reaction from Step A1.7.
- Add 40  $\mu\text{L}$  (0.8X) of resuspended AMPure XP beads to the reaction. Mix well by pipetting up and down. Collect the contents at the bottom of the tube by briefly spinning the tube in a microcentrifuge.
- Incubate at room temperature for 10 minutes. Mix the sample halfway through the incubation by pipetting up and down.
- Place the tube on a magnetic stand until the solution is clear (3-5 minutes). Discard the supernatant without disturbing the beads.
- Add 200  $\mu\text{L}$  of freshly prepared 80% ethanol to the tube while still on the magnetic stand. Wait 30 seconds, then remove and discard the ethanol. Do not remove the tube from the magnetic stand while performing the ethanol wash.
- Repeat the previous wash step.
- Briefly spin the tube and return it to the magnetic stand. Ensure that all residual ethanol is removed at this step.
- Open the cap of the tube while it is on the magnetic stand and allow the beads to air dry for up to 5 minutes.
- Remove the tube from the magnetic stand and add 40  $\mu\text{L}$  of Nuclease-Free Water to the beads. Mix well to resuspend the beads by pipetting up and down. Collect the contents at the bottom of the tube by briefly spinning the tube in a microcentrifuge.
- Incubate at room temperature for 10 minutes. Mix the sample halfway through the incubation by pipetting up and down. Collect the contents at the bottom of the tube by briefly spinning the tube in a microcentrifuge.
- Place the tube on the magnetic stand. Allow the solution to clear and transfer the supernatant containing the eluted DNA to a new 0.2 mL PCR tube.
- Proceed to the next step (PCR Amplification).

 **SAFE STOPPING POINT:** If stopping at this point in the protocol, store the sample at  $-20^{\circ}\text{C}$ .

## Step B: PCR Amplification

Hands-on time: ~30 min | Total time: ~1 hour

### Reagent Preparation

Item	Storage	Handling
2X PCR Mix	-20°C	If frozen, thaw on ice. Finger-tap mix and spin down. Keep on ice.
P7 Primer	-20°C	Thaw at room temperature. Vortex briefly and spin down. Keep on ice.
P5 Primer		
Tris Buffer	-20°C	Bring to room temperature. Vortex and invert mix.
AMPure XP Beads	4°C	
80% Ethanol	Room Temperature	Prepare fresh.

### B1: PCR Amplification

- On ice, combine the following reagents in the order listed below in a 0.2 mL nuclease-free PCR tube:

Amplification Reaction	Volume
Depleted DNA product (Step A2.11)	40 µL
2X PCR Mix	50 µL
P7 Primer	5 µL
P5 Primer	5 µL
Total Volume	100 µL

- Place the reaction in a thermal cycler with a heated lid set to 105°C. Run the following program:

Temperature	Cycle Time	Number of cycles
95°C	2 min	1 cycle
98°C	20 sec	8 cycles*
55°C	30 sec	
72°C	30 sec	
72°C	2 min	1 cycle
4°C	HOLD	

\*The number of PCR cycles may have to adjusted as yield will depend on sample type, library quality and mitochondrial content.

- Proceed immediately to the next step (Bead Cleanup).

### B2: Bead Cleanup

- Add 80 µL (0.8X) of resuspended AMPure XP beads to the reaction. Mix well by pipetting up and down. Collect the contents at the bottom of the tube by briefly spinning the tube in a microcentrifuge.
- Incubate the sample at room temperature for 10 minutes. Mix the sample halfway through the incubation by pipetting up and down.
- Place sample tube on a magnetic stand until the solution is clear (3-5 minutes). Discard the supernatant without disturbing the beads.
- Add 200 µL of freshly prepared 80% ethanol to the tube while still on the magnetic stand. Wait 30 seconds, then remove and discard the ethanol. Do not remove the tube from the magnetic stand while performing the ethanol wash.
- Repeat the previous wash step.
- Briefly spin the tube and return it to the magnetic stand. Ensure that all residual ethanol is removed at this step.

7. Open the cap of the tube while it is on the magnetic stand and allow the beads to air dry for up to 5 minutes.
8. Remove the tube from the magnetic stand and add 30  $\mu$ L of Tris Buffer to the beads. Mix well to resuspend the beads by pipetting up and down. Collect the contents at the bottom of the tube by briefly spinning the tube in a microcentrifuge.
9. Incubate the sample at room temperature for 10 minutes. Mix the sample halfway through the incubation by pipetting up and down. Collect the contents at the bottom of the tube by briefly spinning the tube in a microcentrifuge.
10. Place the tube on the magnetic stand. Allow the solution to clear and transfer the supernatant containing the eluted DNA to a new DNA LoBind tube. This constitutes the depleted DNA library.

 **SAFE STOPPING POINT:** If stopping, store the library at  $-20^{\circ}\text{C}$ .

## Subsequent Steps

Jumpcode Genomics recommends assessing the library yield using a dsDNA-specific fluorescence-based method (such as a Qubit fluorometer) and library size on an Agilent 2100 Bioanalyzer or equivalent instrument before sequencing.

After the second (and final) bead cleanup, most DNA fragments in the depleted library should be larger than 200 bp. If so, the library can be loaded directly on an Illumina sequencer. If a large proportion of fragments are less than 200 bp, it is recommended that a gel-based size selection step be performed to isolate DNA larger than 200 bp in size. The DNA can be loaded on a sequencing instrument after gel purification.

This product is intended for research purposes only.

This product is not intended to be used for therapeutic or diagnostic purposes in humans or animals.

This product is covered by one or more patents, trademarks and/or copyrights owned or controlled by Jumpcode Genomics, Inc. For more information about commercial rights, please email us at [support@jumpcodegenomics.com](mailto:support@jumpcodegenomics.com). While Jumpcode Genomics develops and validates its products for various applications, the use of this product may require the buyer to obtain additional third party intellectual property rights for certain applications.

AMPURE XP<sup>®</sup> is a registered trademark of Beckman Coulter, Inc.

BIOANALYZER<sup>®</sup> is a registered trademark of Agilent Technologies,

Inc. ILLUMINA<sup>®</sup> is a registered trademark of Illumina, Inc.

NEBNext<sup>®</sup> is a registered trademark of New England Biolabs, Inc.

DepleteX<sup>™</sup> is a registered trademark of Jumpcode Genomics, Inc.

Qubit<sup>®</sup> is a registered trademark of Thermo Fisher Scientific, Inc.